

IoT-Based Smart Health-Monitoring Ventilator System for Enhanced Patient Safety

Dinesh C

PG Scholar, Department of Medical Electronics,
Sengunthar Engineering College (Autonomous), Tiruchengode, India
sdineshcd@gmail.com

Kavitha V 

Assistant Professor, Department of Medical Electronics,
Sengunthar Engineering College (Autonomous), Tiruchengode, India
ykavitha.bme@gmail.com

<https://orcid.org/0000-0003-2636-8930>



Publication History

Manuscript Reference No: IJIRAE/RS/Vol.13/Issue03/AEMR26.MRAE10176

Research Article | Open Access | Double-Blind Peer-Reviewed| ArticleID:IJIRAE/RS/Vol.13/Issue03/AEMR26.MRAE10176

Received:22,February 2026, Revised: 01, March 2026, Accepted: 16,March 2026,Published Online: 25, March 2026.

<https://www.ijirae.com/volumes/Vol13/iss-03/95.AEMR26.MRAE10176.pdf>

Article Citation: Dinesh,Kavitha(2026), IoT-Based Smart Health-Monitoring Ventilator System for Enhanced Patient Safety,IJIRAE: International Journal of Innovative Research in Advanced Engineering, Volume 13, Issue 03 of 2026 pages 691-696 **Doi:**><https://doi.org/10.26562/ijirae.2026.v1303.95> **BibTeX Key:** Dinesh@2026IoT-Based

IJIRAE papers should be cited as IJIRAE (International Journal of Innovative Research in Advanced Engineering, AM Publications, India 2025, ISSN 2349-2163, <https://doi.org/10.26562/ijirae.2026.v1303.95> The journal's official abbreviation is IJIRAE. **Orcid:** <https://orcid.org/0009-0004-9398-7488>

About the License: Copyright©2026 copyright by the authors. This article is an open access and license under the terms and conditions of the Creative Commons Attribution (CC BY) license (<https://creativecommons.org/licenses/by/4.0/>).

Abstract: This work tackles the constraints of current low-resource ventilator systems. These systems sometimes lack built-in monitoring for the environment and vital signs, which reduces patient safety and increases the need for using multiple devices. The proposed solution is a smart, affordable health-monitoring ventilator system. It combines temperature, humidity, light, heart rate, blood oxygen levels, and dangerous gas detection into a single automated platform. The system's goal is to provide constant, real-time monitoring. It also seeks to enhance comfort by automatically adjusting fans and lights, according to input from various sensors. The Arduino microcontroller handles both data gathering and control, operating effectively on its own, without needing any outside components. To improve use in both home and clinical settings, the readings are shown immediately on an LCD panel. The aim is to offer a cost-effective, space-saving, and dependable multi-parameter monitoring system, well suited for environments with limited resources. This system's uniqueness comes from merging environmental sensing, biomedical monitoring, and automatic ventilation control into a single, completely integrated, and affordable system.

Keywords: Smart Health Monitoring, Integrated Sensing, Patient Safety, Real-Time Tracking, Low-Cost Design, Automated Ventilation, Biomedical Monitoring.

I. INTRODUCTION

As healthcare organizations increasingly adopt patient-centered, technology-driven models that promote comfort, safety, and real-time decision-making, smart health-monitoring technologies have become increasingly vital. In both home and hospital settings, environments with ventilation require constant monitoring of physiological and environmental factors [1] to maintain the best health outcomes. Traditional ventilation systems usually rely on distinct sensors to measure temperature, humidity, air quality, vital signs, and other important elements. This separation raises costs and maintenance needs, and it also limits access for areas with fewer resources who need reliable and affordable monitoring tools. In modern healthcare, the emphasis on early detection, rapid reaction, and the integration of sensing technologies has led to an increasing need for compact systems. These systems should automate environmental control while also accurately and easily collecting patient health data. The emergence of affordable embedded platforms [2], like Arduino, has enabled the design of smart systems. These systems can combine sensing, computation, and actuation in a compact form. Integrating sensors that measure temperature, humidity, light, heart rate, oxygen levels, and dangerous gases allows for the creation of a multi-parameter system. This system offers thorough monitoring without needing complex external devices. Moreover, this connectivity improves reliability. The system continuously updates and shows important information in real-time [3], allowing caregivers to respond instantly to any unusual findings. In areas with limited medical resources, an independent and affordable device that helps manage the environment and track vital signs could greatly improve patient outcomes. This is because it reduces the time it takes to discover potential health problems. Automated control of ventilation and lighting is a significant step forward in increasing patient comfort and reducing the need for manual changes. The system may automatically control a DC fan and lighting components by using environmental sensors to detect changes in temperature, humidity, or ambient light. This automation lightens the burden on caregivers [4] and helps maintain the right environmental conditions for patients. This is especially important for those who need steady airflow, clean air, or specific lighting to aid their recovery.

Furthermore, the incorporation of biomedical sensors, including infrared-based heartbeat rate modules, SpO detectors, and MQ-2 gas sensors, broadens the system's functionality beyond mere environmental observation. This integration facilitates a comprehensive methodology that simultaneously records internal physiological data and external environmental influences impacting patient health. Displaying all monitored [5] parameters directly on an LCD module significantly improves usability. This design choice eliminates the need for external computers or mobile devices, which makes the system well-suited for remote areas, places with limited resources, or during emergencies. Being able to see real-time data instantly keeps caregivers, patients, and their families in the loop, eliminating the need to wrestle with complicated systems or technical hurdles. This straightforward design facilitates quick implementation when instant monitoring is essential. Think temporary clinics, home-care isolation setups, or medical facilities with limited resources. The work demonstrates how integrated sensing, intelligent control, and economical technology may be incorporated into a single, coherent platform. This platform [6] then improves health management methods. This technology, by combining environmental tracking with vital-sign monitoring and automated actuation, presents a tangible way to boost patient safety and comfort. It's a significant step forward in the development of healthcare technologies that are easier for everyone to use. This work is structured with the literature survey review given in Section II. Section III outlines the methodology, with specific focus on its operability. Results and discussions are in Section IV. Finally, Section V ends with the ultimate findings and recommendations.

II. LITERATURE SURVEY

The recent work on smart health-monitoring systems has increasingly focused on combining environmental and biomedical sensors to improve patient safety and comfort. Recent studies highlight the need for affordable, automated solutions that integrate monitoring vital signs with ventilation management that can adjust to changing conditions. The development of embedded systems and sensor technologies has enabled the creation of small, reliable platforms. These platforms are appropriate for continuous monitoring in both home and clinical settings. This study offers a non-invasive ventilator, complete with several sensors, designed for use in both clinical settings and home telemedicine. It keeps [7] tabs on vital signs, sending them wirelessly for remote monitoring. This provides a patient-centric method for ongoing respiratory assistance, allowing for immediate oversight thanks to built-in communication capabilities. This study provides an automated oxygenation system. It changes airflow based on a patient's state and sends important information through mobile communication. It improves emergency response efforts [8] by controlling oxygen supply and delivering real-time information. This provides a readily available solution for supportive respiratory care, even for those without specialized technical training. This study describes a ventilator that conserves oxygen by adjusting its breathing assistance based on certain physiological measures of the patient. It keeps tabs on crucial health metrics, adjusting home ventilation to work best when resources are tight. This provides [9] a useful option for keeping breathing steady while saving oxygen in hospital settings where supplies are limited. This study explores a learning-based approach to improve how patients and ventilators work together during assisted breathing. The system assesses performance across different situations, showing a considerable improvement in responsiveness. Its goal [10] is to minimize issues stemming from breathing inconsistencies, so contributing to safer and more effective respiratory care, particularly in challenging clinical environments. This study investigates the issues of maintaining stable breathing and heart function during robotic surgery. The text highlights concerns relating to how patients are positioned, airway pressure [11], and the length of surgical procedures. It emphasizes the significance of meticulous monitoring and teamwork to protect patient safety and minimize complications in complex surgical situations. This review underlines the limitations of existing ventilators and presents a portable, cost-effective device ideal for urgent care settings. The system stresses ease of use, built-in sensing [12], and better access for patients with breathing problems. This is especially important in situations when quick deployment and affordability are crucial for appropriate respiratory assistance.

This study studies how intelligent systems can be integrated into ventilators to improve clinical decision-making. This analysis explores how interconnected processing and cloud-based [13] insights can facilitate prompt modifications, lessen the burden of monitoring, and ultimately enhance patient care. The goal is to expand the functionality of current breathing equipment. This study proposes a self-organizing framework designed to manage networked healthcare services. This approach showcases how adaptive [14] coordination can enhance continuous newborn monitoring. By creating responsive service groups, it boosts both flexibility and dependability within dynamic healthcare settings, all while minimizing the need for manual input. This study offers a small negative-pressure ventilator, meant to be both affordable and comfortable. Built with robust materials and equipped [15] with safety measures, this device is designed for ease of use. It provides a viable option for respiratory support in critical situations, tackling issues related to expense, ease of transport, and patient comfort. This study describes the creation of a ventilator system that uses the Internet of Things (IoT) to improve accessibility. The system is designed to help patients [16] in critical situations. It automates breathing support using controlled compression, offering a cost-effective solution. This technique increases access to vital respiratory treatment, especially in areas with limited resources. This study presents a connected paradigm for forecasting ventilator failures in clinical settings. It pinpoints susceptible elements and offers ongoing surveillance [17], alerting users to potential problems as they arise. This approach enhances safety, minimizes operational interruptions, and facilitates proactive upkeep for essential respiratory devices. This study examines how to pick extra monitoring devices to assist active asset tracking in healthcare settings. This method uses a structured priority system [18] to identify equipment that needs constant monitoring. This improves operational awareness and supports better management of vital resources. This study proposes a monitoring system designed to identify early spoiling in stored crops, utilizing gas sensing technology. The system provides constant data gathering and remote monitoring.

This allows [19] facilities to uphold quality standards, minimize waste, and fine-tune environmental factors throughout the extended storage of delicate agricultural goods. This study presents a method for finding loose bolts in ventilation systems, utilizing signals as indicators. This study analyzes how changes in structural behavior can show signs of deterioration. This allows [20] for quicker identification of harmful circumstances and supports better maintenance of important industrial ventilation systems.

III. METHODOLOGY

The methodology describes the whole operational process of the smart health-monitoring ventilator system. It details how data is collected, processed, evaluated, and displayed to assure ongoing patient safety and environmental comfort. The process begins with the simultaneous collection of environmental and biomedical data. This is followed by a methodical signal conditioning phase, which transforms the initial electrical signals into precise digital values. These revised values are subsequently reviewed using programmed decision-making procedures, which control the automatic operation of ventilation and lighting systems. The final processed results are presented to the user via a real-time LCD interface. This structured approach allows for the smooth integration of sensing, processing, control, and display functions. As a result, it enables a completely automated, cost-effective monitoring platform. This platform is designed for reliable home and clinical applications, requiring minimal human involvement.

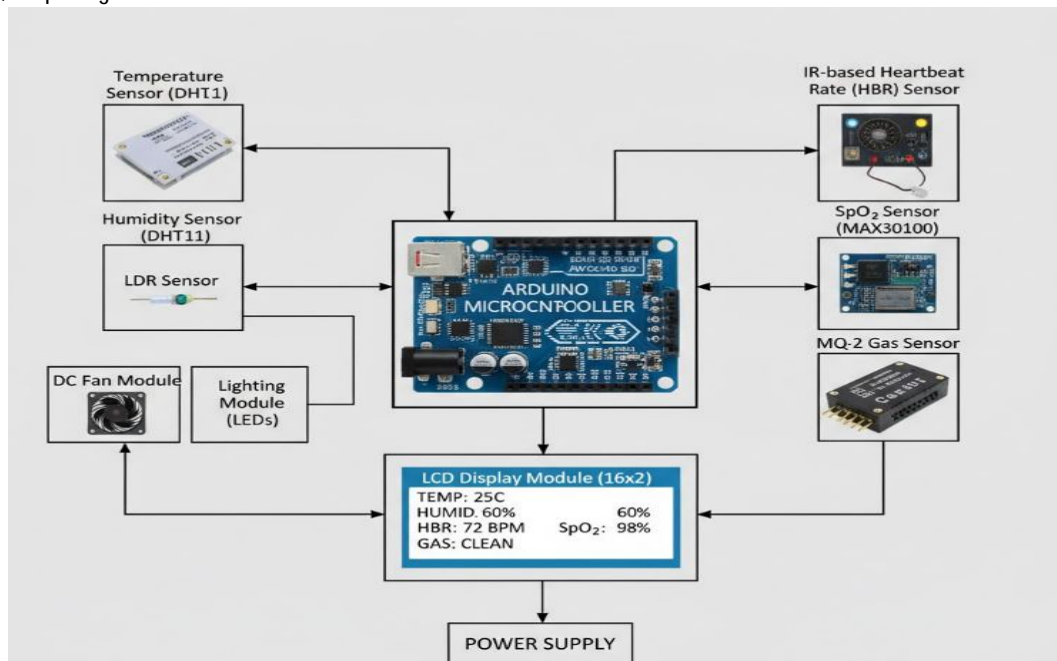


Fig. 1: Block diagram

A. Sensor Data Acquisition

During this stage, all sensors in the system continuously collect real-time environmental and health data, which is necessary for reliable monitoring. The DHT11 sensor monitors temperature and humidity, providing information about the environment's comfort. At the same time, the LDR measures the surrounding light intensity, which is used to adjust lighting. The infrared heartbeat sensor collects biomedical data by detecting pulse changes, while the SpO₂ sensor measures oxygen saturation. At the same time, the MQ-2 gas sensor detects smoke and hazardous gasses, which could be dangerous to patients. The Arduino Uno receives data from each sensor, using either analog or digital pins. This setup allows for continuous and coordinated data collection. The system's automatic monitoring capabilities are built on this multi-parameter acquisition step.

B. Signal Processing and Conditioning

After the raw data is collected by the Arduino, the signal processing phase transforms these electrical outputs into useful, reliable, and interpretable measurements. Analog signals are changed into digital signals by a process called analog-to-digital conversion, which allows for numerical representation of different values. In contrast, digital signals are directly understood by looking at the logical levels produced by sensors. To stabilize the changing waveforms, noise filtering is performed to heartbeat signals. In addition, calibration algorithms are used to assure the accuracy of SpO₂ and gas sensors. To provide accurate measurements in different environments, temperature, humidity, and light data are handled using programmed conversion procedures. The Arduino constantly fine-tunes and verifies every parameter, removing any inconsistencies that can compromise the system's dependability. This phase guarantees the controller gets data that's not just clean, but also precise and easy to understand, making it ready for immediate operation and display.

C. Decision-Making and Automation Control

In this phase, the Arduino assesses the processed data against predetermined thresholds and circumstances, which allows the system to respond automatically. Should the temperature or humidity levels surpass predefined thresholds, the controller springs into action. It then uses the L293D driver to control the DC fan, ensuring a consistent and comfortable airflow.

As soon as the light-dependent resistor (LDR) senses a drop in surrounding light levels, the Arduino takes action, activating the DC light to brighten the area. The monitoring of vital signs uses various systems to identify unusual heart rates, low oxygen levels, or high concentrations of gases. These systems then trigger quick automatic responses. These automated systems work without human involvement, allowing them to function continuously, even in areas with limited resources. The automation framework is the system's basic intelligence, delivering timely corrective measures to preserve patient comfort and safety.

D. Real-Time Display and User Output

Ultimately, the Arduino sends all the processed data to the LCD module. This allows for the real-time display of temperature, humidity, light levels, heart rate, SpO₂ %, and the status of gas concentrations. The display refreshes periodically, so users can always see the latest system data, no need for any outside gadgets. This interface prioritizes straightforwardness and instant understanding, enabling caregivers and patients to swiftly evaluate both environmental and biological factors. The constant display on the device also promotes transparency in how the system works. This allows for early discovery of problems and helps users make educated decisions. This stage completes the monitoring process by turning internal system data into easily available, real-time information. This information can then be used in both home and clinical settings.

IV. RESULT AND DISCUSSION

The smart, low-cost health-monitoring ventilator system's results show that combining environmental sensing, biological monitoring, and automated actuation creates a reliable, unified platform. This platform is suited for use in both home and clinical settings. The system's performance during testing showed consistent results. It accurately recorded temperature, humidity, light intensity, heart rate, SpO₂ levels, and gas concentrations. This confirmed that the chosen sensors were well-suited to the project's goals. The DHT11 sensor offered responsive environmental data, accurately reflecting changes in the surrounding conditions. This allowed the Arduino to alter the ventilation system in real time. Similarly, the light-dependent resistor (LDR) accurately monitored changes in the surrounding light. This triggered the direct current (DC) light to turn on if the light level went below the set threshold. The results verified the automatic environmental-control components worked well, showing that the system could maintain pleasant conditions without needing human intervention. To show the consistency of the sensor outputs, a representative numerical dataset was recorded during the system's evaluation. The following table summarizes the readings taken throughout the prototype's stable operation. It shows ambient variables, vital signs, and gas concentration levels measured in a controlled setting.

Table 1: Performance analysis

Temp (°C)	Humidity (%)	Light (LDR)	Heart Rate (BPM)	SpO ₂ (%)	Gas (MQ-2)
29	63	210	78	97	182
30	61	198	80	96	190
31	64	220	79	97	185
28	60	205	76	98	178
29	62	215	77	97	181

The collected data shows that the sensor's reaction is consistent across different measurements. Environmental readings alter predictably with temperature and humidity. At the same time, the light-dependent resistor (LDR) values demonstrate the precise measurement of light levels. The biomedical sensing results were also impressive, with the infrared heartbeat sensor and the SpO₂ module providing reliable physiological data over the extended monitoring durations. The heartbeat sensor effectively recorded pulse signals using optical changes. After filtering and processing, it delivered accurate and reliable beats-per-minute data. The SpO₂ sensor provided continuous measurements of oxygen saturation, and its precision was satisfactory for the low-cost hardware used. This made it useful for early detection of unusual breathing patterns or signs of patient decline. The MQ-2 gas sensor quickly detected changes in smoke and gas levels, offering an extra safety feature when dangerous concentrations were present. The Arduino's automated control logic was crucial for connecting sensor data to immediate actions. The decision-making algorithms correctly identified when thresholds were exceeded and then took the required steps. These included turning on the fan when temperatures climbed and altering the illumination depending on the LDR measurements. The results demonstrated that the system's built-in control model could operate independently, while yet maintaining logical and responsive behavior. Moreover, the transitions between different actuation states were smooth. This showed that the L293D motor driver and the related hardware were set up correctly, able to handle the switching requirements without any delays or instability. The system's architecture is considered robust and suitable for continuous operation because of the stable interaction between sensing, processing, and actuation components. The LCD module provided complete transparency by displaying all processed parameters in real time, constantly updating output values throughout the testing duration. This feature allowed for a visual check of each reading's accuracy, giving users immediate information on changes in their environment and body. The interface's clarity and ease of use demonstrated that the system could be reliably controlled by people with no technical experience. The combined data and analysis demonstrate that the suggested system works well as a compact, integrated, and cost-effective monitoring solution. The capacity to monitor numerous environmental and biological variables, coupled with precise processing capabilities and the ability to initiate automated actions, has considerable promise for application in resource-constrained settings. These settings often require constant monitoring, yet lack the financial means to procure traditional instrumentation.

V. CONCLUSION

This work reveals the successful construction of a combined smart health-monitoring ventilator system. This system integrates environmental sensing, vital-sign monitoring, and automated actuation into a single, cost-effective platform. The system's holistic approach to patient comfort and safety is achieved by combining data on temperature, humidity, light intensity, heart rate, oxygen saturation, and gas levels. Automated control of fans and lighting significantly improves usability. This reduces the need for constant manual adjustments, making the system ideal for home care, clinical settings, and areas with limited resources. Its small size and use of easily sourced parts underscore its usefulness and low cost. This makes it a good choice for ongoing monitoring in situations where standard equipment isn't available or doesn't quite cut it. This study's main contribution is the creation of a unified and automated system, which aims to improve patient management by making it safer and more efficient. Future research could focus on improving sensor accuracy, adding wireless connectivity for remote health monitoring, expanding the system to include more biomedical data, and optimizing the user interface for improved interaction. Moreover, further enhancements could examine decision-making models based on machine learning. This would allow for predictive insights and adaptive control. These guidelines could improve the system, making it more intelligent, scalable, and adaptable for health monitoring, which would allow for wider use.

REFERENCES

1. A. Aziz et al., "Revolutionizing Critical Care: A Smart Positive Pressure Based Non-Invasive Ventilator with Real-time IoT Health Monitoring System," 2023 IEEE 6th International Conference on Knowledge Innovation and Invention (ICKII), Sapporo, Japan, 2023, pp. 1-6, <https://doi.org/10.1109/ICKII58656.2023.10332616>
2. N. N, M. G. Urs, N. N, K. K. N and S. T, "Smart Ventilator for Affordable Health Monitoring System," 2025 International Conference on Intelligent and Innovative Technologies in Computing, Electrical and Electronics (IITCEE), Bangalore, India, 2025, pp. 1-6, <https://doi.org/10.1109/IITCEE64140.2025.10915464>
3. M. Menniti, G. Oliva, F. Laganà, M. G. Bianco, A. S. Fiorillo and S. A. Pullano, "Portable Non-Invasive Ventilator for Homecare and Patients Monitoring System," 2023 IEEE International Symposium on Medical Measurements and Applications (MeMeA), Jeju, Korea, Republic of, 2023, pp. 1-5, <https://doi.org/10.1109/MeMeA57477.2023.10171872>
4. F. Ullah, M. J. Khan, Q. Arsalan, J. Khattak, U. A. Siddiqui and A. A. Siddiqui, "IoT Platform for Remote Monitoring and Controlling Small-scale Ventilator for SAR Patient," 2023 15th International Conference on Innovations in Information Technology (IIT), Al Ain, United Arab Emirates, 2023, pp. 202-207, <https://doi.org/10.1109/IIT59782.2023.10366493>
5. S. Ren, X. Wang, M. Cai, Y. Shi, T. Wang and Z. Luo, "Design of a Multi-Parameter Fusion Sensor and System for Respiratory Monitoring of Mechanically Ventilated Patients in the ICU," in IEEE Journal of Biomedical and Health Informatics, vol. 29, no. 2, pp. 923-934, Feb. 2025, <https://doi.org/10.1109/JBHI.2024.3471822>
6. B. Jeeva, P. U. Managoli, M. Patil, M. V. Marigoli and C. Monisha, "Design and Development of Low-Cost Mechanical Ventilator with Remote Patient Monitoring," 2023 7th International Conference on Design Innovation for 3 Cs Compute Communicate Control (ICDI3C), Karnataka, India, 2023, pp. 295-298, <https://doi.org/10.1109/ICDI3C61568.2023.00066>
7. M. Menniti, F. Laganà, M. G. Bianco, G. Oliva, A. S. Fiorillo and S. A. Pullano, "Sensorized Non-Invasive Ventilator for Clinical Applications in Telemedicine," 2024 IEEE International Symposium on Medical Measurements and Applications (MeMeA), Eindhoven, Netherlands, 2024, pp. 1-5, <https://doi.org/10.1109/MeMeA60663.2024.10596712>
8. R. Faiz, N. N. Alam, M. A. Araf, A. Saha and M. H. Imam, "Design and Implementation of Regulated Oxygenation Based Ventilation System with Feedback Mechanism," 2023 3rd International Conference on Robotics, Electrical and Signal Processing Techniques (ICREST), Dhaka, Bangladesh, 2023, pp. 249-253, <https://doi.org/10.1109/ICREST57604.2023.10070056>
9. M. S. Rahman Akash, R. Faiz, N. N. Alam and M. H. Imam, "Automatic Oxygen Flow Regulated Non- Invasive Ventilator with Vital Sign Monitoring System," 2024 11th International Conference on Information Technology, Computer, and Electrical Engineering (ICITACEE), Semarang, Indonesia, 2024, pp. 163-168, <https://doi.org/10.1109/ICITACEE62763.2024.10761953>
10. L. Hao et al., "Improving Patient-Ventilator Synchrony During Pressure Support Ventilation Based on Reinforcement Learning Algorithm," in IEEE Journal of Biomedical and Health Informatics, vol. 29, no. 8, pp. 5974-5982, Aug. 2025, <https://doi.org/10.1109/JBHI.2025.3551670>
11. S. Saranya, T. Sreelekha and J. Deepthi, "Anesthesia for Robotic Surgery: Navigating Hemodynamic, Respiratory and Positioning Challenges," 2025 IEEE 6th International Conference in Robotics and Manufacturing Automation (ROMA), Selangor, Malaysia, 2025, pp. 96-100, <https://doi.org/10.1109/ROMA66616.2025.11155267>
12. H. Gaur, S. Yadav, Shashikant, A. Shahin and M. Shahid, "Review On Design and Performance of the Medical Ventilators," 2023 International Conference on Power, Instrumentation, Energy and Control (PIECON), Aligarh, India, 2023, pp. 1-5, <https://doi.org/10.1109/PIECON56912.2023.10085815>
13. L. Valentine C J, A. Ahmed B, E. Raja and U. PA, "Enabling Augmented Intelligence Using Gen AI in Mechanical Ventilators," 2024 International Conference on Smart Electronics and Communication Systems (ISENSE), Kottayam, India, 2024, pp. 1-6, <https://doi.org/10.1109/ISENSE63713.2024.10872334>
14. S. Poornima and A. Immanuel, "Self-Organizing Microservice Composition for IoT-Enabled Neonatal Monitoring," 2025 International Conference on Advances in Modern Age Technologies for Health and Engineering Science (AMATHE), Shivamogga, India, 2025, pp. 1-5, <https://doi.org/10.1109/AMATHE65477.2025.11081365>

15. S. S. M. Gaben et al., "ExoventQ: A Novel Low-Cost Portable Negative Pressure Ventilator Design and Implementation," in IEEE Access, vol. 12, pp. 61828-61847, 2024, <https://doi.org/10.1109/ACCESS.2024.3390566>.
16. C. P. Mallikarjuna Gowda, B. M. Bellishree, V. Janhavi, M. C. Prakruthi and R. Pawar, "Venti-Smart: Crafting Smart Ventilators with IoT Technology," 2024 International Conference on Knowledge Engineering and Communication Systems (ICKECS), Chikkaballapur, India, 2024, pp. 1-6, <https://doi.org/10.1109/ICKECS61492.2024.10617223>
17. O. Manchadi, Z. E. O. Dehbi, F. -E. Ben-Bouazza, A. Edder, I. Tafala and B. Jioudi, "IoT-Powered Predictive Maintenance Framework for ICU Ventilators," 2024 International Conference on Intelligent Systems and Computer Vision (ISCV), Fez, Morocco, 2024, pp. 1-7, <https://doi.org/10.1109/ISCV60512.2024.10620162>
18. S. Suakanto, E. Nuryatno, A. Z. Hafizhah, W. A. Nurtrisha, T. A. Nugroho and F. Wahyudin, "Development of Selection Method for Additional Devices to Supporting Active Monitoring of Healthcare Asset," 2023 International Conference on Advancement in Data Science, E-learning and Information System (ICADEIS), Bali, Indonesia, 2023, pp. 1-8, <https://doi.org/10.1109/ICADEIS58666.2023.10270841>
19. B. Correia, R. Thorn, R. D. Hancock, D. Nelson, D. Reynolds and J. A. Covington, "TuberSense: Industrial application of gas sensing as a tool for monitoring crop spoilage," 2025 IEEE Sensors Applications Symposium (SAS), Newcastle, United Kingdom, 2025, pp. 1-5, <https://doi.org/10.1109/SAS65169.2025.11105202>.
20. J. Zhang, Y. Shi, C. Chen and L. Zheng, "Fault Diagnosis of Loose Anchor Bolt of Coal Mine Ventilator Based on EMI," 2025 IEEE 7th International Conference on Communications, Information System and Computer Engineering (CISCE), Guangzhou, China, 2025, pp. 745-750, <https://doi.org/10.1109/CISCE65916.2025.11065048>.